Aquilant
A HC2I Group Company

securAcath®

REMOVAL

- If insertion site is dry or firm, apply saline soaked gauze to the site for 3-5minutes, this will soften the skin aiding easier removal.
- Catheter can be withdrawn and haemostasis achieved before or after securAcath is removed (as per local protocol)

Step 1

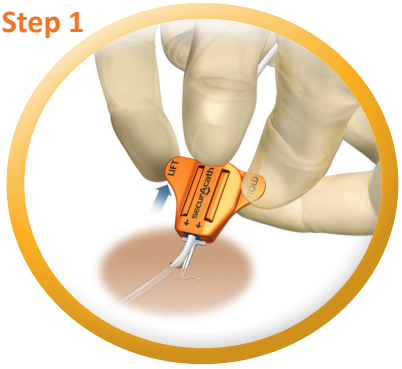

- Grip the HOLD tab with thumb and finger of one hand to stabilise device and securement feet beneath the skin
- Pry upward at the edge of LIFT tab with index finger tip of other hand and thumb placed at center to release cover from base

Step 2

- Completely detach cover from base

FOLD OPTION

Can be used with or without catheter in place

Step 3

- Gently pull skin above SecurAcath taut
- Fold wings downward to bring feet together under the skin

Step 4

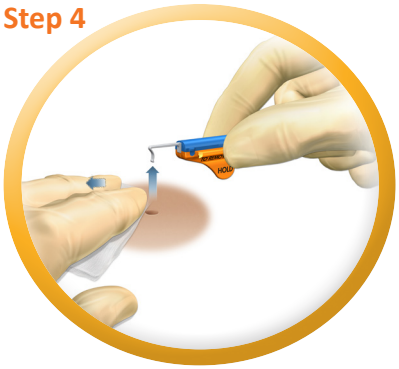

- Hold folded base horizontal to skin
- Use swift, deliberate upward motion to remove

SPLIT OPTION

Catheter must be removed prior to using this method

Step 3

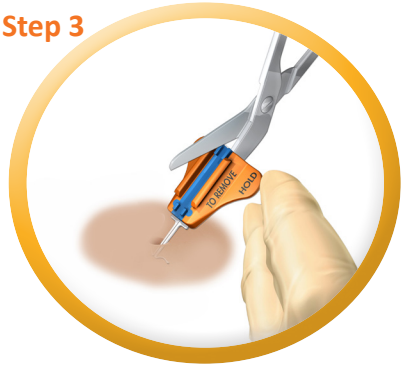

- Use a blunt tip scissors to cut base completely in half lengthwise along the groove

Step 4

- Gently pull skin above SecurAcath taut
- The flexible securement feet are shaped like an “L” with the feet extending 5mm to each side of the insertion site

Step 5

- Turn blue edge upward and use a swift, deliberate upward motion to remove each foot separately

Distributed By Aquilant
Aquilant House, Unit B1-B2 Bond Close, Kingsland Business Park,Basingstoke, Hampshire, RG24 8PZ, United Kingdom
T: +44 (0) 1256 306 506 E: contactus@aquilantservices.com

Interrad Medical
181 Cheshire Lane, Suite 100
Plymouth, MN 55441 USA
+1.763.225.6699
www.securacath.com

interrad MEDICAL

securAcath YouTube

SecurAcath® app!
Download on the App Store
GET IT ON Google play